

acumed[®]

Total Wrist Fusion Plating System


+ acumed® | Total Wrist Fusion Plating System

The Total Wrist Fusion Plating System contains five plates with both innovative and traditional designs. Specifically, four of the five plates are positioned on the second metacarpal which may reduce extensor tendon irritation. Additionally, the fifth plate is placed on the third metacarpal and developed for use with a proximal row carpectomy. All plates have a 15° dorsal bend, established as a balance between anatomic resting position, hand function, and grip strength.

STANDARD AND SMALL PLATES

Left and right specific plates with two size variations for placement on the second metacarpal which may reduce extensor tendon irritation.

Convergent distal screw construct is designed to increase resistance to pullout.

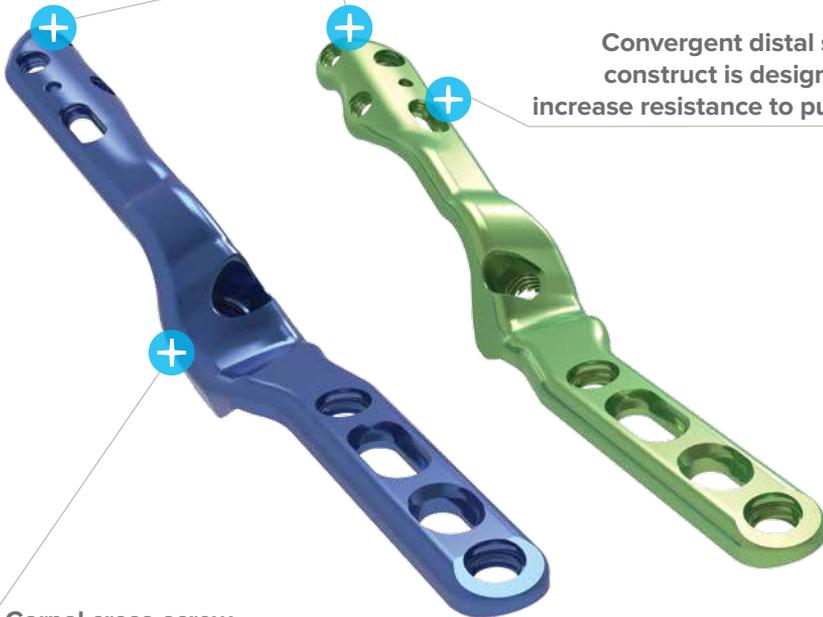

Carpal cross-screw designed to offer additional implant stability.

SAVELOCK COMPRESSION SLEEVE


The SaveLock Compression Sleeve engages screw head threads, reducing the plate to the bone by preventing the screw from locking into the plate until the SaveLock Compression Sleeve is disengaged.



NEUTRAL PLATE

2.3 mm Hexalobe Multiscrews for locking and nonlocking applications utilizing a T6 Hexalobe interface.

Neutral plate placed on the third metacarpal designed for use with a proximal row carpectomy.

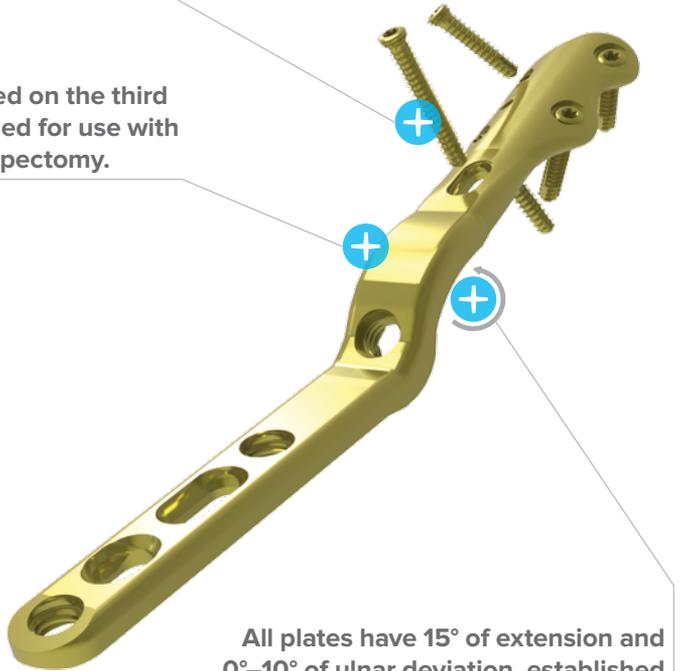

All plates have 15° of extension and 0°–10° of ulnar deviation, established as a balance between anatomic resting position, hand function, and grip strength.

For more information, please visit: acumed.net



HNW40-08-A

Effective: 5/2014

© 2014 Acumed® LLC

Acumed® Headquarters
5885 NW Cornelius Pass Road
Hillsboro, OR 97124

Office: 888.627.9957

Fax: 503.520.9618

acumed.net

These materials contain information about products that may or may not be available in any particular country or may be available under different trademarks in different countries. The products may be approved or cleared by governmental regulatory organizations for sale or use with different indications or restrictions in different countries. Products may not be approved for use in all countries. Nothing contained on these materials should be construed as a promotion or solicitation for any product or for the use of any product in a particular way which is not authorized under the laws and regulations of the country where the reader is located. Specific questions physicians may have about the availability and use of the products described on these materials should be directed to their particular local sales representative. Specific questions patients may have about the use of the products described in these materials or the appropriateness for their own conditions should be directed to their own physician.

Acumed® is a registered trademark of Acumed, LLC.